


MASTERFLEX® REGLO 78018-10

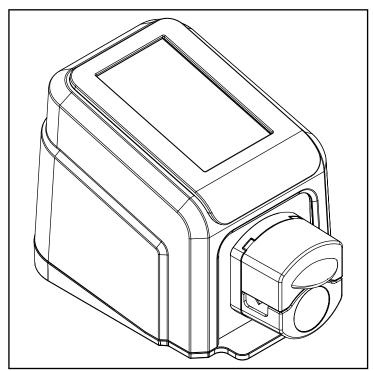

MASTERFLEX® REGLO 78018-40

Masterflex®

(US & Canada only) Toll Free 1-800-MASTERFLEX • 1-800-637-3739 (Outside US & Canada) 1-847-549-7600 • 1-847-381-7050 www.masterflex.com • techinfo@masterflex.com OPERATING MANUAL:

REGLO DIGITAL PUMP DRIVES WITH ADVANCED CONNECTIVITY

Model Nos.

78018-10
78018-12
78018-14
78018-20
78018-22
78018-24
78018-40
78018-42

A-1299-5201 Edition 01 © 2019 Cole-Parmer Instrument Company. All rights reserved. **Masterflex**[®] is a registered trademark of the Cole-Parmer Instrument Company. Trademarks bearing the ® symbol in this publication are registered in the US and in other countries.

PUMP FOR LIQUIDS ORIGINAL INSTRUCTIONS

Table of Contents

SECTION 1: INTRODUCTION	1-1
Safe Operation	
About the REGLO	
Package Contents	
Available Models	
Peristaltic Cassette Models	
Peristaltic Miniflex Models	
Non-Peristaltic Pump Models	2-1
SECTION 2: BASIC SETUP & SETTINGS	2-2
Touchscreen Icons	3-1
Before Starting the Drive	
Switching on the Drive	
Loading Tubing	
Cassette Models	
Miniflex Models	
Priming the Pump Drive	
Tube Calibration	
Tube Calibration Screen	
Settings	
Language Settings	
Device Name	
Setting the Time	
Setting the Date	
WI-FI	
Ethernet Settings	
Screen Saver	
Display Brightness	
Auto Start Dispense & Batch Completion Alerts	
Analog Output	
Device Information	
SECTION 3: OPERATION	
Mode Selection Screen	
Continuous Mode	
Continuous Mode Run Screen Continuous Mode Operation	
Saving Continuous Mode Settings as a New Program	

Time Mode	
Time Mode Run Screen	
Time Mode Edit Screen	
Time Mode Operation	
Saving Time Mode Settings as a New Program	
Volume Mode	
Volume Mode Run Screen	
Volume Mode Edit Screen	
Volume Dispense Mode Operation	
Saving Volume Mode Settings as a New Program.	
Anti-Drip	
Volume Record	
Remote Mode	
Remote Mode Run Screen	
Using MasterflexLive [™]	
Analog Input	
Saving Remote Mode Settings as a New Program	
Custom Program Modes	
Adding a New Program: Continuous Mode	
Adding a New Program: Time Mode	
Adding a New Program: Volume Mode	
Adding a New Program: Remote Mode Using Program Modes	
Editing a Program	
Deleting a Program.	
SECTION 4: SERVICE & MAINTENANCE	
Cleaning the Pump Drive	
Software & Firmware Updates	
Restore Factory Settings	
DB-25 Electrical Connections	
Miniflex Pump Head Replacement	
Troubleshooting	
Error Definitions	
Accessories	
REGLO Accessories	
Cassettes	
Color-Coded Three-Stop Tubing	
Specifications	
Technical Assistance	
Product Return	
Warranty	
Disposal	

SECTION 1: INTRODUCTION

SAFE OPERATION

The REGLO Digital Pump Drive with Advanced Connectivity is designed for pumping and dispensing applications in laboratory and process environments. Confirm that the pump drive is operated only in the manner specified in this operating manual and that safe work practices and Good Laboratory Practice (GLP) are followed. Misuse of the pump drive may compromise built-in safety protections and result in injury and/ or damage to equipment. Do not operate the pump drive with water on the surface of the touchscreen.

The following Safety Symbols are used in this documentation:



CAUTION: Risk of Danger. Consult Operating Manual for nature of hazard and corrective actions.

CAUTION: Risk of crushing. Keep fingers away from the rotor while the pump is in operation. Stop pump before loading or unloading tubing.

CAUTION: Hot Surface. Do not touch.

CAUTION: Risk of electric shock. Consult Operating Manual for nature of hazard and corrective actions.

ABOUT THE REGLO

The REGLO Digital Pump Drive with Advanced Connectivity offers precise flow control and highly accurate fluid dispensing ideal for laboratory, process, and field use. All REGLO precision drives include a highly accurate, maintenance-free motor and an easy to navigate touchscreen that makes setup and operation easier than ever. The REGLO range features Ethernet and Wi-Fi connections for web-based remote control and monitoring using the MasterflexLive[™] website (see <u>www.masterflex.com</u>), and remote analog control and monitoring through the pump drive's DB-25 female connection port.

Package Contents

- Pump Drive
- 24 VDC Desktop Power Supply Set
- Quick Start Guide
- Flash Drive Containing the Operating Manual

NOTE: Please check the package and its contents for any visible signs of damage. If any damage is found please contact Technical Assistance immediately (see "<u>Technical Assistance</u>" on page 3-48).

Model	Description	Pump Type	RPM (MAX)	Channels	Rollers	Cartridge/Heads
78018-10	2CH6RLR	Peristaltic	160	2	6	Click'n'go
78018-12	2CH8RLR	Peristaltic	160	2	8	Click'n'go
78018-14	2CH12RLR	Peristaltic	160	2	12	Click'n'go
78018-20	4CH6RLR	Peristaltic	160	4	6	Click'n'go
78018-22	4CH8RLR	Peristaltic	160	4	8	Click'n'go
78018-24	4CH12RLR	Peristaltic	160	4	12	Click'n'go
78018-40	Miniflex	Peristaltic	350	1	3	Miniflex Pump (Single Channel)
78018-42	Miniflex	Peristaltic	350	2	3	Miniflex Pump (Dual Channel)
78018-50	Gear Pump	Gear	5000	1	-	A-mount Gear Pump
78018-60	Piston Pump	Piston	1800	1	-	FMI Piston Head

Available Models

Peristaltic Cassette Models

Features:

- A 5-inch multi-language touchscreen display providing easy access to user-defined operation parameters and direct readouts of pump operation data, including pump speed, flow rates, flow direction, and batch totals.
- Volume, Time, Continuous, and Remote modes for quick and easy operation.
- User selectable dispense volumes, tube diameters, flow rates, pump speeds, and run times.
- Anti-drip control.
- Brushless, maintenance-free motor offering ±0.1% speed control accuracy with a turndown ratio greater than 1500:1.
- Easy pump priming and tube calibration.
- Peristaltic Cassette models have a maximum speed of 160 RPM and flow rate capacities that range from 0.001 mL/min through to 68 mL/min (depending on the model and tubing size selected).
- Takes MS/CA Click'n'go tube cassettes for easy loading and removal.
- Can take up to two channels or up to four channels (depending on the model) allowing simultaneous multiple fluid channels on the same pump.

Peristaltic Miniflex Models

The REGLO is available in two non-cassette pump head models (78018-40 and 78018-42). The REGLO Miniflex Digital Pump Drives feature:


- An easy to load pump head that accepts continuous lengths of tubing for clean flow paths.
- Automatic tubing retention that makes tube loading quick and easy.
- Tool free tube replacement.
- Available with one or two tube channels.
- A maximum speed of 350 RPM and flow rate capacities ranging from 0.006 mL/min to 324 mL/min (depending on the model and tubing size selected).

Go to <u>www.masterflex.com</u> for further information.

Non-Peristaltic Pump Models

The REGLO is also available in a Gear Pump model (78018-50) and a Piston Pump model (78018-60). Go to <u>www.masterflex.com</u> for further information.

SECTION 2: BASIC SETUP & SETTINGS

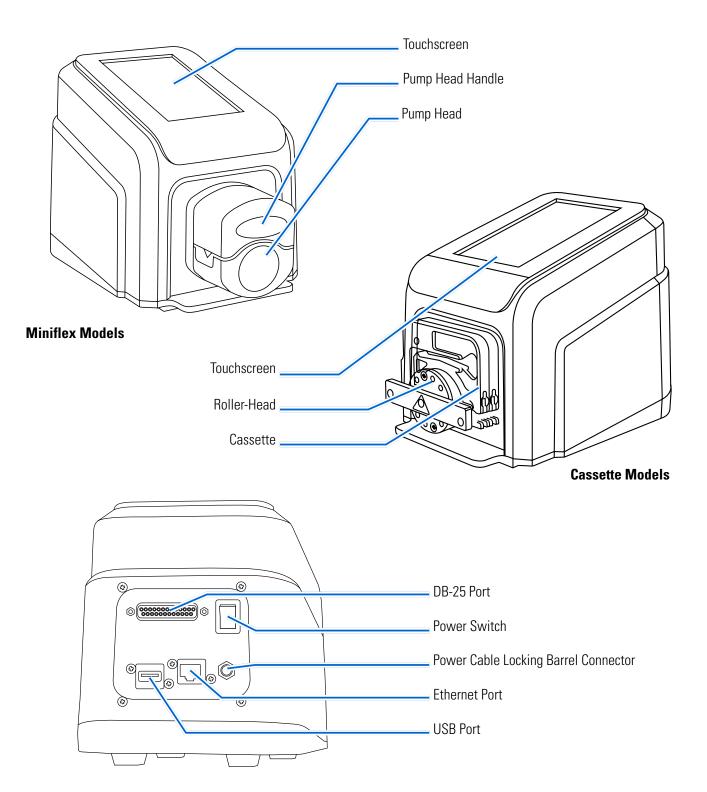

TOUCHSCREEN ICONS

	Calibrate	>>	Prime
¢,	Calibration Complete		Program
\sim	Clockwise		Ramp Down
× ~	Close/Cancel		Ramp Up
~	Confirm		Record Volume
⇒	Continuous	Ð	Remote
\sim	Counterclockwise	Ð	Reset
×	Delete	ē 🔒	Screen Lock
$\Diamond $	Display Brightness	•	Settings
	Edit		Start
	Language		Stop
÷	New Program	Ō	Time
11	Pause	E	Volume

BEFORE STARTING THE DRIVE



CAUTION: Do not block the rear panel of the pump drive. The power switch must always be easy to access and the power cord must always be easy to disconnect.



CAUTION: Turn the drive off before removing or installing tubing. Fingers or loose clothing could get caught in the drive mechanism.



CAUTION: The power cord set supplied with your pump drive meets the requirements of the country where you purchased the pump drive. If you use the pump drive in another country, you must use a power cord set that meets the requirements of that country.



CAUTION: If the product is not used in the manner specified in the instructions, the protection provided by the equipment may be impaired.

- Ensure the pump drive is mounted on a flat surface.
- Ensure adequate air flow around the pump drive and ensure that the ambient air temperature does not exceed 104° F (40° C).
- Tubing should be clean and routed so that bend radii are at a minimum of four (4) times the outside tube diameter and are as short as possible.
- Use the appropriate tube diameter for the required flow rate and viscosity.
- Recalibrate tubing regularly to maintain the best flow rate accuracy (for further information see "<u>Tube</u> <u>Calibration</u>" on page 3-8).
- For tubing selection and compatibility go to <u>www.masterflex.com</u>.
- Remove the pump drive's power cord from the mains power outlet when cleaning or performing maintenance on the drive.

SWITCHING ON THE DRIVE

- 1. Plug in and securely fasten the supplied 24 VDC desktop power supply to the power cable barrel connector located at the rear of the drive.
- 2. Plug the opposite end of the power cable into a mains power outlet.
- 3. Switch the drive on using the power switch located at the rear of the drive. **NOTE:** The drive takes approximately two minutes to complete start-up.

- On the initial start-up the Language Settings screen will be displayed. A language must be selected before pump operation (for further information see "Language Settings" on page 3-10).
- Following the initial start-up all subsequent start-ups will revert to the mode of operation screen previously in use.
- After 30 minutes of inactivity the REGLO will enter sleep mode and the display will turn off. Tapping the touchscreen will reactivate the drive. To enable (default) or disable the screen saver see "<u>Screen Saver</u>" on page 3-12.

LOADING TUBING


Cassette Models



CAUTION: Turn the drive off before removing or installing tubing. Fingers or loose clothing could get caught in the drive mechanism.

The REGLO Cassette models use MS/CA Click'n'go cassettes for easy loading and removal, and to allow for tubes with different diameters and materials to be used on the same roller-head. Cassettes are also available with pressure levers. For further information see "<u>Cassettes</u>" on page 3-44 and "<u>Color-Coded Three-Stop</u> <u>Tubing</u>" on page 3-45.

- Check to confirm that the rollers are clean and free of defects.
- Tubing should be clean and routed so that the bend radii are at a minimum of four (4) times the outside tube diameter and are as short as possible.
- Use the appropriate tube diameter for the required flow rate and viscosity.
- Recalibrate tubing regularly to maintain the best flow rate accuracy (for further information see "<u>Tube</u> <u>Calibration</u>" on page 3-8).
- After installing new tubing the pump should be run for 20-30 minutes to properly condition the tubing and increase dispense accuracy (for further information see "**to condition new tubing**" below).

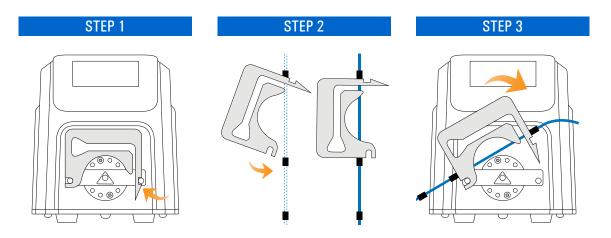

- 1. Remove the cassette by lightly pressing the fixing-tongue while simultaneously lifting the cassette.
- 2. Insert the tubing into the cassette:
 - a. Insert the first stopper of the color-coded three-stop tubing into the cassette's front tube channel.
 - b. Allow the tubing to hang freely to prevent twisting.
 - c. Insert the second stopper of the tubing into the cassette's rear tube channel.
- 3. Replace the cassette onto the roller-head.

To condition new tubing:

After installing new tubing the pump should be run for 20-30 minutes at full rpm (160 rpm). This is recommended to properly condition new tubing and to increase dispense accuracy. If required, the pump can be run dry while conditioning.

- 1. Switch the drive on using the power switch located at the rear of the drive. **NOTE:** The drive takes approximately two minutes to complete start-up.
- 2. Tap CONTINUOUS from the Mode Selection screen. The Continuous Mode Run screen will be displayed.
- 3. Select the flow rate and flow units:
 - a. Tap FLOW RATE. The Flow Rate screen will be displayed.
 - b. Tap UNITS. The Flow Units screen will be displayed.
 - c. Tap RPM.
 - d. Tap CONFIRM **v** to return to the Flow Rate screen.
 - e. Tap FLOW RATE to select field and then enter 160 using the onscreen keypad.
 - f. Tap CONFIRM 🔽 to save and return to the Continuous Mode screen.
- 4. Tap START ► . The drive will commence operation.
- 5. Allow the pump to run for 20-30 minutes before tapping STOP ■. The tube is now conditioned and ready for priming, calibration, and use.


- Once the tube has been loaded and conditioned the new tube's size will need to be selected from the Tube Size screen. The Tube Size screen can be accessed from the Continuous Mode Run screen or from either of the Volume or Time Mode Edit screens.
- It is recommended that you calibrate new tubes to ensure accurate flow rate and fluid dispensing (for further information see "<u>Tube Calibration</u>" on page 3-8).
- When the pump is idle it is recommended that you release pressure from the tubing to protect it from unnecessary strain and prolong its service life. **To release tube pressure:** Press the cassette's fixing-tongue and raise the cassette slightly so that the tubing is released from the roller-head. **CAUTION**: Siphoning Effect: When pressure is released from the tubing, fluid can flow back to the reservoir.
- When using new tubing it is possible that the pump will not prime and/or will not dispense fluid (depending on the type of tubing used). If this occurs, it is recommended that you wet the tubing and then run the pump with the tubing for approximately 20-30 minutes.
- For applications with a high differential pressure (>1 bar), the use of a cassette with a pressure lever is recommended.

Miniflex Models



CAUTION: Turn the drive off before removing or installing tubing. Fingers or loose clothing could get caught in the drive mechanism.

- Check to ensure that the rollers are clean and free of defects.
- Tubing should be clean and routed so that bend radii are at a minimum of four (4) times the outside tube diameter and are as short as possible.
- Use the appropriate tube diameter for the required flow rate and viscosity.
- Regularly recalibrate tubing to maintain the best accuracy of flow rates (for further information see "<u>Tube</u> <u>Calibration</u>" on page 3-8).
- After installing new tubing the pump should be run for 20-30 minutes to properly condition the tubing and increase dispense accuracy (for further information see "**to condition new tubing**" below).

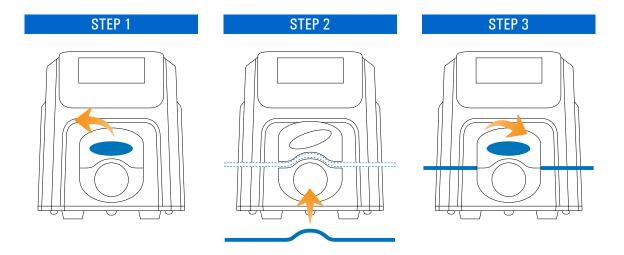

- 1. Turn the pump head handle counterclockwise to raise the upper section of the pump head.
- 2. Place the tube into the opening, ensuring that the tube is:
 - a. Completely inside the pump head.
 - b. Seated over the roller-head.
 - c. Sitting in the V-shaped grooves located on either side of the pump head.
- 3. Turn the pump head handle clockwise to close the pump head.

To condition new Miniflex tubing:

After installing new tubing the pump should be run for 20-30 minutes at full rpm (350 rpm). This is recommended to properly condition new tubing and to increase dispense accuracy. If required, the pump can be run dry while conditioning.

- 1. Switch the drive on using the power switch located at the rear of the drive. **NOTE:** The drive takes approximately two minutes to complete start-up.
- 2. Tap CONTINUOUS from the Mode Selection screen. The Continuous Mode Run screen will be displayed.
- 3. Select the flow rate and flow units:
 - a. Tap FLOW RATE. The Flow Rate screen will be displayed.
 - b. Tap UNITS. The Flow Units screen will be displayed.
 - c. Tap RPM.
 - d. Tap CONFIRM **v** to return to the Flow Rate screen.
 - e. Tap FLOW RATE to select field and then enter 350 using the onscreen keypad.
 - f. Tap CONFIRM 🔽 to save and return to the Continuous Mode screen.
- 4. Tap START ► . The drive will commence operation.
- 5. Allow the pump to run for 20-30 minutes before tapping STOP ■. The tube is now conditioned and ready for priming, calibration, and use.

- Once the tube has been loaded and conditioned the new tube's size will need to be selected from the Tube Size screen. The Tube Size screen can be accessed from the Continuous Mode Run screen or from either of the Volume or Time Mode Edit screens.
- It is recommended that you calibrate new tubes to ensure accurate flow rate and fluid dispensing (for further information see "<u>Tube Calibration</u>" on page 3-8).
- When using new tubing it is possible that the pump will not prime and/or will not dispense fluid (depending on the type of tubing used). If this occurs, it is recommended that you wet the tubing and then run the pump with the tubing for approximately 20-30 minutes.

PRIMING THE PUMP DRIVE

It is recommended that you prime the pump drive before use. Priming the pump draws fluid through the tubing and eliminates air pockets from the system.




CAUTION: Keep fingers away from the rotor while the pump is in operation. Stop the pump before loading or unloading tubing.



CAUTION: Turn the drive off before removing or installing tubing. Fingers or loose clothing could get caught in the drive mechanism.

Example Flow System

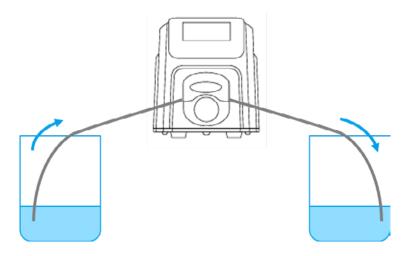


To prime the pump drive:

- 1. Insert the appropriate tubing into the pump head (for further information see "Loading Tubing" on page 3-3).
- 2. Insert the tube inlet into the supply fluid.
- 3. Insert the tube outlet into an appropriate container.
- 4. Switch the drive on using the power switch located at the rear of the drive.
- 5. Navigate to the Continuous, Time or Volume Mode screens.
- 6. Press and hold PRIME >> until no bubbles are visible in the tubing. Priming will stop when PRIME >> is released.

TUBE CALIBRATION

Tube calibration should be performed whenever fluids, flow rate or tubing is changed to ensure accurate dispensing of fluids. Tube calibration can be accessed from the Continuous Mode Run screen or from either of the Volume or Time Mode Edit screens.

Tube Calibration Screen

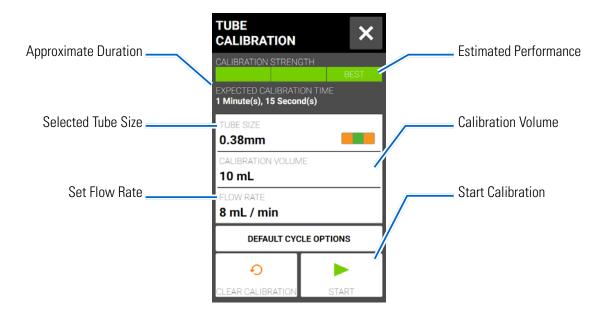

General Preparation:

- Confirm the correct tubing has been selected and is properly loaded into the pump drive (for further information see "Loading Tubing" on page 3-3).
- Confirm all fluids and containers are ready.

To calibrate tubing:


- 1. Insert the tube inlet into the supply fluid.
- 2. Insert the tube outlet into a suitable container. **NOTE:** The container should be graduated or placed on a scale for increased accuracy. If using a scale, an acceptable weight to volume conversion for water is: 1 gram = 1 mL.
- 3. Switch the drive on using the power switch located at the rear of the drive.
- 4. Navigate to the Continuous, Time or Volume Mode screens.
- 5. Tap DIRECTION to select either clockwise
 r or counterclockwise
 flow direction.
- 6. If required, Tap START ► and allow the pump to run for approximately 20-30 minutes. This step is recommended to properly condition new tubing and to increase calibration accuracy. **NOTE:** If required, the pump can be run dry while conditioning the tube.
- 7. Press and hold PRIME **>>** to prime the pump. Priming will stop when PRIME **>>** is released.

- 8. Tap SIZE from the Continuous Mode screen or tap EDIT 🖌 and then SIZE if either the Volume or Time Mode screen is displayed. The Tube Size screen will be displayed.
 - a. Select the desired tube size from the available options or SCROLL ♥ and tap CUSTOM to enter a custom tube size.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to previous screen.
- 9. Tap CALIBRATE . The Tube Calibration screen will be displayed.
- 10. Tap CALIBRATION VOLUME. The Calibration Volume screen will be displayed.
 - a. Enter the desired calibration volume using the onscreen keypad. **NOTE:** The default volume or greater will ensure the best calibration.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the previous screen.
- 11. Tap FLOW RATE. The Calibration Flow Rate screen will be displayed.
 - a. Enter the desired flow rate using the onscreen keypad.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the previous screen. **NOTE:** The drive will adjust the displayed flow rate after calibration is complete.
- 12. Tap START > to begin calibration. **NOTE:** Calibration progress will be displayed on the touchscreen.
- 13. When calibration is complete use the onscreen keypad to enter the measured volume of fluid from the tube outlet container.
- 14. Tap CONFIRM 🔽 to complete calibration and return to the previous mode screen. Calibration Complete 🗇 should now be displayed to indicate that calibration has been completed for the current tube size, tube volume, and flow rate.

- The estimated accuracy for the selected calibration settings is shown in the Calibration Strength bar on the Tube Calibration screen. Calibration accuracy can be improved by using a larger calibration volume and/or altering the flow rate.
- Calibration settings are retained and transferred to other mode screens when entering or leaving the Tube Calibration screen.
- If the drive is stopped during calibration the calibration will be discarded and the previous mode screen will be displayed. Empty the container before restarting the procedure.
- Calibration time at the maximum allowable flow rate (default max flow rate) is approximately 10 seconds. Calibration time at the minimum allowable flow rate (approximately 4% of the maximum flow rate) is 4 minutes. Select a custom tube size for other tubing sizes or lower flow rates (see step 8 above).
- Minimum and maximum flow rates will change after calibration due to a recalculation of the volume of fluid per pump revolution.
- The best results are obtained after tubing has been run in the pump for approximately 20-30 minutes.
- Steps 9–14 can be repeated as necessary to optimize the accuracy of the tubing calibration.

SETTINGS

The Settings screen allows access to basic configuration settings. The Settings screen is accessed by tapping SETTINGS 🖸 from any of the mode screens.

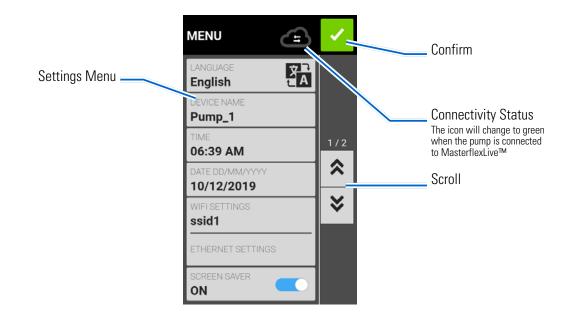

Language Settings

The REGLO Digital Pump Drive can display English, French, German, Italian, and Spanish languages. The default display language is English.

To change the display language:

- 1. Tap SETTINGS 🖸 from any of the mode screens. The Settings screen will be displayed.
- 2. Tap LANGUAGE.
- 3. Select the desired language from the available list.
- 4. Tap CONFIRM 🔽 to save the new language selection.

Device Name

Individual names can be assigned to each REGLO Digital Pump Drive to make identification easier when using more than one pump.

To assign a pump drive name:

- 1. Tap SETTINGS O from any of the mode screens. The Settings screen will be displayed.
- 2. Tap DEVICE NAME. The Device Name screen will be displayed.
- 3. Enter the desired pump name using the onscreen keypad (up to 8 characters).
- 4. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes.

Setting the Time

To change the time:

- 1. Tap SETTINGS 🖸 from any of the mode screens. The Settings screen will be displayed.
- 2. Tap TIME.
- 3. Select either 12-HOUR or 24-HOUR time.
- 4. Tap HH to select hours and enter the desired time using the onscreen keypad.
- 5. Tap MM to select minutes and enter the desired time using the onscreen keypad.
- 6. If using 12-HOUR time, tap AM/PM to select either AM or PM.
- 7. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes.

Setting the Date

To change the date:

- 1. Tap SETTINGS 🖸 from any of the mode screens. The Settings screen will be displayed.
- 2. Tap DATE.
- 3. Select the desired date format (either month/day/year or day/month/year).
- 4. Tap the desired MONTH, DAY or YEAR field to select and then enter the date using the onscreen keypad.
- 5. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes.

WI-FI

The REGLO can connect to a network using Wi-Fi and Ethernet connections.

NOTE:

- The Ethernet connection will take priority if both Wi-Fi and Ethernet are used simultaneously.
- The REGLO supports WEP, WPA, WPA2, and None (open) Wi-Fi security protocols.

To select a Wi-Fi network:

- 1. Tap SETTINGS 🖸 from any of the mode screens. The Settings screen will be displayed.
- 2. Tap WIFI SETTINGS. The Wi-Fi Settings screen will be displayed.
- 3. If required, tap the WIFI toggle to select either ON or OFF.
- 4. Tap the desired Wi-Fi network from the available list.
- 5. If required, enter the network PASSWORD using the onscreen keypad.
- 6. Tap CONNECT to join the network or CANCEL to cancel.
- 7. Tap CONFIRM 🔽 to return to the Settings screen.

To remove a Wi-Fi network:

- 1. Tap SETTINGS O from any of the mode screens. The Settings screen will be displayed.
- 2. Tap WIFI SETTINGS. The WIFI Settings screen will be displayed.
- 3. Locate the desired Wi-Fi network and tap REMOVE WIFI 🖬 .
- 4. Tap REMOVE to remove the network or CANCEL to discard changes.
- 5. Tap CONFIRM 🔽 to return to the Settings screen.

Ethernet Settings

The REGLO can connect to a network using Wi-Fi and Ethernet connections.

NOTE:

- Confirm that the Ethernet cable is securely attached to the Ethernet port at the rear of the pump drive.
- The Ethernet connection will take priority if both Wi-Fi and Ethernet are used simultaneously.

To configure Ethernet settings:

- 1. Tap SETTINGS 🖸 from any of the mode screens. The Settings screen will be displayed.
- 2. Tap ETHERNET SETTINGS. The Ethernet Settings screen will be displayed.
- 3. Tap DHCP to automatically configure IP settings or STATIC to manually edit settings using the onscreen keypad.
- 4. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes.

Screen Saver

The REGLO has a screen saver to help extend the display life of the touchscreen. After 30 minutes of inactivity the REGLO will enter sleep mode and the display will turn off. Tapping the touchscreen will reactivate the drive.

To enable or disable the screen saver:

- 1. Tap SETTINGS 🖸 from any of the mode screens. The Settings screen will be displayed.
- 2. Tap the SCREEN SAVER toggle to select either ON or OFF.

Display Brightness

To adjust the display brightness:

- 1. Tap SETTINGS 🖸 from any of the mode screens. The Settings screen will be displayed.
- 3. Use the slider to adjust the touchscreen brightness to the desired level.

Auto Start

The REGLO has an auto start that will resume pump operation when power is restored after a power outage.

To enable auto start:

- 1. Tap SETTINGS O from any of the mode screens. The Settings screen will be displayed.
- 3. Tap the AUTO START toggle to select either ON or OFF.

Dispense & Batch Completion Alerts

When Sound Dispense is enabled a short beep will sound at the completion of each pump dispense. When Sound Batch is enabled a single long beep will sound at the completion of each batch cycle.

To enable or disable the dispense completion alert:

- 1. Tap SETTINGS O from any of the mode screens. The Settings screen will be displayed.
- 3. Tap the SOUND DISPENSE toggle to select either ON or OFF.

To enable or disable the batch cycle completion alert:

- 1. Tap SETTINGS O from any of the mode screens. The Settings screen will be displayed.
- 3. Tap the SOUND BATCH toggle to select either ON or OFF.

Analog Output

The REGLO supports and controls analog output through the pump drive's 25-pin connection (for further information see "DB-25 Electrical Connections" on page 3-40.

- 1. Tap SETTINGS 🖸 from any of the mode screens. The Settings screen will be displayed.
- 3. Tap ANALOG OUTPUT. The Analog Output screen will be displayed.
- 4. Tap the desired analog output type from the available list.
- 5. If using either ANALOG: VOLTAGE or ANALOG: CURRENT:
 - a. Tap EDIT 🖊 . The Analog: Voltage or Analog: Current Edit screen will be displayed.
 - b. Select the desired current or voltage operating range from the available list.
 - c. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes. The Analog Output screen will be displayed.
- 6. Tap CONFIRM 🗹 .

Device Information

The Device Information screen provides pump drive details such as MAC address, IP address, software version, build date, and firmware version. Factory reset and updates are also accessed from the Device Information screen.

To access the Device Information screen:

- 1. Tap SETTINGS O from any of the mode screens. The Settings screen will be displayed.
- 3. Tap DEVICE INFORMATION. The Device Information screen will be displayed.

See also "Software & Firmware Updates" on page 3-39, and "Restore Factory Settings" on page 3-39.

SECTION 3: OPERATION



WARNING: Tube breakage may result in fluid being sprayed from the pump. Use appropriate measures to protect operator and equipment.



CAUTION: Keep fingers away from the rotor while the pump is in operation. Stop the pump before loading or unloading tubing.




CAUTION: Hot Surface. Do not touch.

CAUTION: To avoid electrical shock, the power cord protective grounding conductor must be connected to ground. Not for operation in wet locations as defined by EN61010-1.

MODE SELECTION SCREEN

The Mode Selection screen allows access to the drive's four basic operation modes (CONTINUOUS, TIME, VOLUME, and REMOTE) as well as the New Program screen and user defined programs. The Mode Selection screen can be accessed from any of the mode screens by tapping the MODE NAME BANNER.

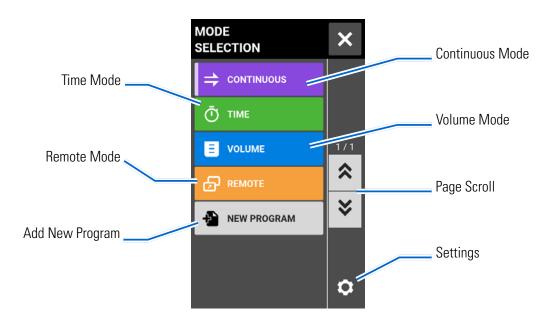


Tap the desired mode or program to access individual mode or program screens.

CONTINUOUS MODE

In Continuous Mode the pump will operate at a selected rpm and/or flow rate until stopped by the user.

Continuous Mode Run Screen

The Continuous Mode Run screen is accessed by selecting CONTINUOUS from the Mode Selection screen.

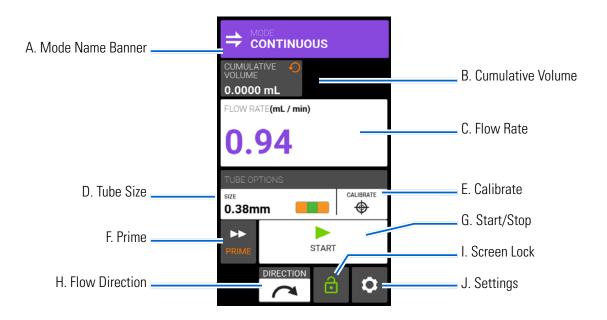

- A. MODE NAME BANNER: Tap the Mode Name Banner to return to the Mode Selection screen.
- B. CUMULATIVE VOLUME: Displays the current cumulative volume of fluid that has been pumped. **To** reset the cumulative volume: Press and hold CUMULATIVE VOLUME RESET ••• until the display changes to zero.
- C. FLOW RATE: Displays the current flow rate in the unit of measurement selected by the user. Tap to access the Flow Rate screen.
- D. SIZE: Tap to access the Tube Size screen.
- E. CALIBRATE: Tap to access the Calibration screen (for further information see "<u>Tube Calibration</u>" on page 3-8). Once calibration has been completed for the current tube size Calibration Complete ***** will be displayed.
- F. PRIME: Press and hold to prime the pump drive (for further information see "<u>Priming the Pump Drive</u>" on page 3-7).
- G. START/STOP: Tap START to begin operation. Once operation has commenced STOP is will be displayed.
- H. FLOW DIRECTION: Tap DIRECTION to select either clockwise 🥂 or counterclockwise 🎮 .

- J. SETTINGS: Tap to access the Settings screen (for further information see "Settings" on page 3-10).

Continuous Mode Operation

General Preparation:

- Confirm the correct tubing has been selected and is properly loaded into the pump drive (for further information see "Loading Tubing" on page 3-3).
- Confirm all fluids and containers are ready.
- Switch the drive on using the power switch located at the rear of the drive. **NOTE:** The touchscreen display will revert to the previously used operation mode.
- Confirm that the tubing has been calibrated by checking that Calibration Complete \$\$\$\$ is displayed on the Continuous Mode Run screen (for further information see "<u>Tube Calibration</u>" on page 3-8).
- If required, prime the pump before operation (for further information see "<u>Priming the Pump Drive</u>" on page 3-7).

To operate the pump in Continuous Mode:

- 1. Tap CONTINUOUS from the Mode Selection screen. The Continuous Mode Run screen will be displayed.
- 2. If required, Press and hold CUMULATIVE VOLUME RESET \bigcirc to reset the display to zero.
- 3. Select the desired flow rate and flow units:
 - a. Tap FLOW RATE to access the Flow Rate screen.
 - b. Tap UNITS to access the Flow Units screen and select the desired flow unit from the available list.
 - c. Tap CONFIRM 🗹 to save or CANCEL 🗙 to discard changes and return to the Flow Rate screen.
 - d. Tap FLOW and enter the desired flow rate using the onscreen keypad.
 - e. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Continuous Mode screen.
- 4. Tap SIZE. The Tube Size screen will be displayed.
 - a. Select the desired tube size from the available list or SCROLL imes and tap CUSTOM to enter a custom tube size using the onscreen keypad.
 - b. Tap CONFIRM ✓ to save or CANCEL × to discard changes and return to the Continuous Mode Run screen.
- 5. If required, tap CALIBRATE to calibrate the pump for the selected tube and flow rate.
- 6. Tap DIRECTION to select either clockwise
 r or counterclockwise
 flow direction.
- 7. Tap START ▶ . The drive will commence operation at the flow rate and direction shown.
- 8. Tap STOP when the drive operation is no longer required. **NOTE:** In Continuous Mode the drive will continue to operate at the displayed flow rate and direction until stopped.

Saving Continuous Mode Settings as a New Program

Changes made to mode parameters can be saved as a new program for easier access to frequently used settings.

To save mode parameters to a new program:

- 1. If required, edit the Continuous Mode settings as desired.
- 2. Tap MODE NAME BANNER to return to the Mode Selection screen.
- 4. Tap CONTINUOUS. The Continuous New Program screen will be displayed with the last settings used in the Continuous Mode.
- 5. Tap PROGRAM1. If required, delete the characters using the back arrow on the onscreen keypad and then enter the desired program name (up to 8 characters).
- 6. Tap CONFIRM to save or DELETE to cancel.


- Once saved, new programs are added in alphabetical order to the bottom of the Mode Selection screen.

TIME MODE

In Time Mode the pump will operate at a selected rpm and/or flow rate for a selected time and/or batch total. At the completion of the selected time or batch total the pump will automatically stop.

Time Mode Run Screen

The Time Mode Run screen is accessed by selecting TIME from the Mode Selection screen.

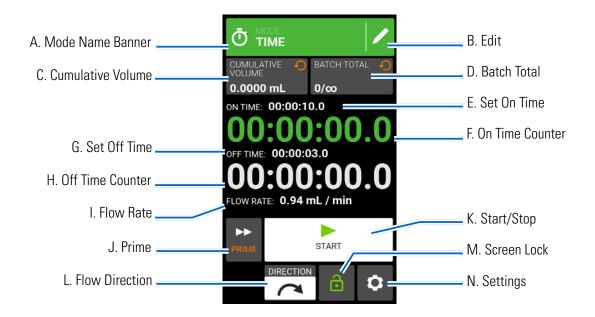

- A. MODE NAME BANNER: Tap the Mode Name Banner to return to the Mode Selection screen.
- B. EDIT: Tap to access the Time Mode Edit screen. From the Time Mode Edit screen changes can be made to flow rate, flow units, tube size, tube calibration, on time, off time, and batch total.
- C. CUMULATIVE VOLUME: Displays the current Cumulative Volume of fluid that has been pumped. **To reset the cumulative volume:** Press and hold CUMULATIVE VOLUME RESET \bigcirc until the display changes to zero.
- D. BATCH TOTAL: Displays the number of dispenses that have been completed in the current batch. **To reset the batch total:** Press and hold BATCH RESET until the display changes to zero.
- E. SET ON TIME: Displays the set dispense operation time.
- F. ON TIME COUNTER: Displays a countdown of the set dispense time during operation.
- G. SET OFF TIME: Displays the set duration of time the pump pauses between each dispense operation.
- H. OFF TIME COUNTER: Displays a countdown of the set off time during operation.
- I. FLOW RATE: Displays the current flow rate in the unit of measurement selected by the user.
- J. PRIME: Press and hold to prime the pump drive (for further information see "<u>Priming the Pump Drive</u>" on page 3-7).

- K. START/STOP/PAUSE: During operation, the display will change from START ► to PAUSE II STOP/ RESET .
- L. FLOW DIRECTION: Tap DIRECTION to select either clockwise
 or counterclockwise
 flow direction.
- M. SCREEN LOCK: Locking the screen disables all touchscreen functions. **To lock the screen:** Press and hold UNLOCKED i until the icon changes to LOCKED i and a red border appears around the screen. **To unlock the screen:** Press and hold LOCKED i until the icon changes to UNLOCKED i.
- N. SETTINGS: Tap to access the Settings screen (for further information see "Settings" on page 3-10).

Time Mode Edit Screen



Time Mode Operation

General Preparation:

- Confirm the correct tubing has been selected and is properly loaded into the pump drive (for further information see "Loading Tubing" on page 3-3).
- Confirm all fluids and containers are ready.
- Switch the drive on using the power switch located at the rear of the drive. **NOTE:** The touchscreen display will revert to the previously used operation mode.
- Confirm that the tubing has been calibrated by checking that Calibration Complete 🛷 is displayed on the Time Mode Edit screen (for further information see "<u>Tube Calibration</u>" on page 3-8).
- If required, prime the pump before operation (for further information see "<u>Priming the Pump Drive</u>" on page 3-7).

To operate the pump in Time Mode:

- 1. Tap TIME from the Mode Selection screen. The Time Mode Run screen will be displayed.
- 2. Tap EDIT 🖌 to access the Time Mode Edit screen.
- 3. Tap ON TIME to set the amount of time for each pump operation. The On Time Edit screen will be displayed.
 - a. Tap HR, MIN, SEC or TENTHS and enter the desired time using the onscreen keypad.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Time Mode Edit screen.
- 4. Tap OFF TIME to set the amount of time the pump will pause between each operation. The Off Time Edit screen will be displayed. **NOTE:** If the off time is set to 0 (zero) the pump drive will require a start input (from either the touchscreen or a wired input) to start the next dispense.
 - a. Tap HR, MIN, SEC or TENTHS and enter the desired time using the onscreen keypad.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Time Mode Edit screen.
- 5. Tap FLOW RATE. The Flow Rate Edit screen will be displayed.
 - a. Tap UNITS to access the Flow Units screen and select the desired flow unit from the available list.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the previous screen.
 - c. Tap FLOW and enter the desired flow rate using the onscreen keypad.
 - d. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Time Mode Edit screen.
- 6. Tap SIZE. The Tube Size screen will be displayed.

 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Time Mode Edit screen.
- 7. Tap BATCH TOTAL to adjust the number of dispenses in each batch cycle. The Batch Total screen will be displayed.
 - a. Enter the desired number of dispenses in a batch using the onscreen keypad. **NOTE:** If required, tap INFINITE **oo** to select an infinite number of dispense cycles. If infinite is selected, the pump will run continuously.
 - b. Tap CONFIRM ✓ to save or CANCEL × to discard changes and return to the Time Mode Edit screen.
- 8. Tap CONFIRM 🔽 to return to the Time Dispense Mode Run screen.
- 9. Tap DIRECTION to select either clockwise
 r or counterclockwise
 flow direction.
- 10. Tap START ► . The pump will now operate until the batch total is completed or until PAUSE **II** or STOP **■** is tapped.
- 11. If required, adjustments can be made to any of the Time Mode option settings during operation. To make any adjustments:

- a. Tap PAUSE **II** and then repeat steps 2–9 above.
- b. Tap CONTINUE > to complete the pump operation once the desired changes have been made.

Saving Time Mode Settings as a New Program

Changes made to mode parameters can be saved as a new program for easier access to frequently used settings.

To save mode parameters to a new program:

- 1. If required, edit the Time Mode settings as desired.
- 2. Tap MODE NAME BANNER to return to the Mode Selection screen.
- 4. Tap TIME. The Time New Program screen will be displayed with the last settings used in the Time Mode.
- 5. Tap PROGRAM1. If required, delete the characters using the back arrow on the onscreen keypad and then enter the desired program name (up to 8 characters).
- 6. Tap CONFIRM to save or DELETE to cancel.


- Once saved, new programs are added in alphabetical order to the bottom of the Mode Selection screen.

VOLUME MODE

In Volume Mode the pump will operate at a selected rpm and/or flow rate until a selected volume of fluid has been pumped. When the selected volume has been pumped the drive will automatically stop.

Volume Mode Run Screen


The Volume Mode Run screen is accessed by selecting VOLUME from the Mode Selection screen.

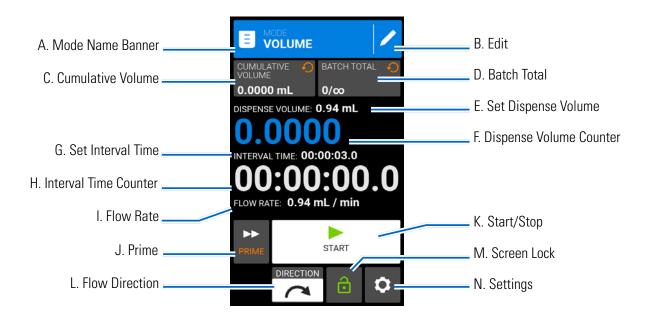

- A. MODE NAME BANNER: Tap the Mode Name Banner to return to the Mode Selection screen.
- B. EDIT: Tap to access the Volume Mode Edit screen. From the Volume Mode Edit screen adjustments can be made to dispense volume, interval time, flow rate, tube options, anti-drip functions, calibration and batch total. **NOTE:** Edit is inactive during operation.
- C. CUMULATIVE VOLUME: Displays the current Cumulative Volume of fluid that has been pumped. **To reset the cumulative volume:** Press and hold CUMULATIVE VOLUME RESET ••• until the display changes to zero.
- D. BATCH TOTAL: Displays the number of dispenses that have been completed in the current batch. **To reset the batch total:** Press and hold BATCH RESET \bigcirc until the display changes to zero.
- E. SET DISPENSE VOLUME: Displays the selected volume of fluid for dispensing.
- F. DISPENSE VOLUME COUNTER: Displays a countdown of the fluid volume during operation.
- G. SET INTERVAL TIME: Displays the set time the pump pauses between dispenses.
- H. INTERVAL TIME COUNTER: Displays a countdown of the set interval time during operation.
- I. FLOW RATE: Displays the current flow rate in the unit of measurement selected by the user.

- J. PRIME: Press and hold to prime the pump drive (for further information see "<u>Priming the Pump Drive</u>" on page 3-7).
- K. START/STOP/PAUSE: During operation, the display will change from START ► to PAUSE STOP/ RESET .
- L. FLOW DIRECTION: Tap DIRECTION to select either clockwise
 or counterclockwise
 flow direction.
- M. SCREEN LOCK: Locking the screen disables all touchscreen functions. **To lock the screen:** Press and hold UNLOCKED i until the icon changes to LOCKED i and a red border appears around the screen. **To unlock the screen:** Press and hold LOCKED i until the icon changes to UNLOCKED i.
- N. SETTINGS: Tap to access the Settings screen (for further information see "Settings" on page 3-10).

Volume Mode Edit Screen

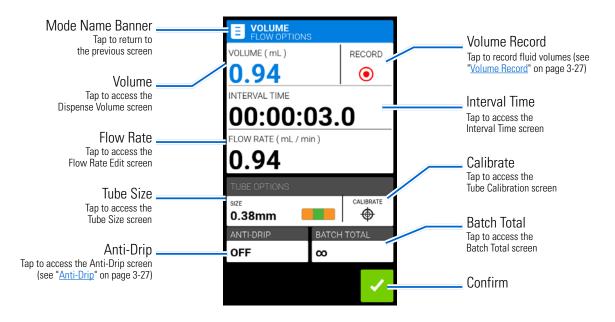

Volume Dispense Mode Operation

General Preparation:

- Confirm the correct tubing has been selected and is properly loaded into the pump drive (for further information see "Loading Tubing" on page 3-3).
- Confirm all fluids and containers are ready.
- Switch the drive on using the power switch located at the rear of the drive. **NOTE:** The touchscreen display will revert to the previously used operation mode.
- Confirm that the tubing has been calibrated by checking that Calibration Complete \$\$\$\$ is displayed on the Volume Mode Edit screen (for further information see "<u>Tube Calibration</u>" on page 3-8).

• If required, prime the pump before operation (for further information see "<u>Priming the Pump Drive</u>" on page 3-7).

To operate the pump in Volume Mode:

- 1. Tap VOLUME from the Mode Selection screen. The Volume Mode Run screen will be displayed.
- 2. Tap EDIT 🖌 to access the Volume Mode Edit screen.
- 3. Tap VOLUME. The Dispense Volume screen will be displayed.
 - a. Tap VOLUME and enter the desired volume using the onscreen keypad. **NOTE:** If the volume of fluid is unknown the pump drive can record fluid dispense volumes (for further information see "<u>Volume Record</u>" on page 3-27).
 - b. Tap RAMP UP \checkmark to set the time the pump takes to reach full flow rate (between 0 and 60 seconds) using the onscreen keypad.
 - c. Tap RAMP DOWN **to** set the time the pump takes to stop at the end of each dispense operation (between 0 and 60 seconds) using the onscreen keypad.
 - d. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Volume Mode Edit screen.
- 4. Tap INTERVAL TIME to set the amount of time the pump will pause between each operation. The Interval Time screen will be displayed. **NOTE:** If the interval time is set to 0 (zero) the pump drive will require a start input (from either the touchscreen or a wired input) to start the next dispense.
 - a. Tap HR, MIN, SEC or TENTHS and enter the desired time using the onscreen keypad.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Volume Mode Edit screen.
- 5. Tap FLOW RATE. The Flow Rate Edit screen will be displayed.
 - a. Tap UNITS to access the Flow Units screen and select the desired flow unit from the available list.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the previous screen.
 - c. Tap FLOW and enter the desired flow rate using the onscreen keypad.
 - d. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Volume Mode Edit screen.
- 6. Tap SIZE. The Tube Size screen will be displayed.
 - a. Select the desired tube size from the available list or SCROLL 孝 and tap CUSTOM to enter a custom tube size using the onscreen keypad.
 - b. Tap CONFIRM ✓ to save or CANCEL × to discard changes and return to the Volume Mode Edit screen.
- 7. Tap BATCH TOTAL to adjust the number of dispenses in each batch cycle. The Batch Total screen will be displayed.
 - a. Enter the desired number of dispenses in a batch using the onscreen keypad. **NOTE:** If required, tap INFINITE **oo** to select an infinite number of dispense cycles. If infinite is selected, the pump will run continuously.

- b. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Volume Mode Edit screen.
- 8. If required, tap ANTI-DRIP. The Anti-Drip screen will be displayed (for further information see "<u>Anti-Drip</u>" on page 3-27).
 - a. Tap ON or OFF to enable or disable the Anti-Drip feature.
 - b. If enabled, enter the desired degrees of reverse rotation using the onscreen keypad. **NOTE:** Typical values range from 5 to 45 degrees.
 - c. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Volume Mode Edit screen.
- 9. Tap CONFIRM 🗹 to return to the Volume Mode Run screen.
- 10. Tap DIRECTION to select either clockwise
 r or counterclockwise
 flow direction.
- 11. Tap START ▶. The pump will now operate until the batch total is completed or until PAUSE II or STOP is tapped.
- 12. If required, adjustments can be made to any of the Volume Mode option settings during operation. To make any adjustments:
 - a. Tap PAUSE **II** and then repeat steps 2–10 above.
 - b. Tap CONTINUE > to complete the pump operation once the desired changes have been made.

Saving Volume Mode Settings as a New Program

Changes made to mode parameters can be saved as a new program for easier access to frequently used settings.

To save mode parameters to a new program:

- 1. If required, edit the Volume Mode settings as desired.
- 2. Tap MODE NAME BANNER to return to the Mode Selection screen.
- 3. Tap NEW PROGRAM. **NOTE:** If NEW PROGRAM is not displayed on the Mode Selection screen tap SCROLL imes to view additional pages.
- 4. Tap VOLUME. The Volume New Program screen will be displayed with the last settings used in the Volume Mode.
- 5. Tap PROGRAM1. If required, delete the characters using the back arrow on the onscreen keypad and then enter the desired program name (up to 8 characters).
- 6. Tap CONFIRM to save or DELETE to cancel.

- Once saved, new programs are added in alphabetical order to the bottom of the Mode Selection screen.

Anti-Drip

The Anti-Drip feature minimizes drips after fluid has been dispensed by reversing the pump direction to draw fluid back from the end of the tubing. Fluid drip can be caused by numerous factors, including tube size, tube orientation, and the viscosity of the fluid.

To enable or disable the Anti-Drip feature:

- 1. Tap VOLUME from the Mode Selection screen. The Volume Mode screen will be displayed.
- 2. Tap EDIT 🖊 .
- 3. Tap ANTI-DRIP. The Anti-Drip screen will be displayed.
- 4. Tap ON or OFF to enable or disable ANTI-DRIP.
- 5. If enabled, enter the desired degrees of reverse rotation using the onscreen keypad. **NOTE:** Typical values range from 5 to 45 degrees.
- 6. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Volume Mode screen.

Volume Record

The Volume Record feature can be used to record unknown fluid volumes.

General Preparation:

- Confirm the correct tubing has been selected and is properly loaded into the pump drive (for further information see "Loading Tubing" on page 3-3).
- Confirm all fluids and containers are ready.
- Confirm that the tubing has been calibrated by checking that Calibration Complete 🌮 is displayed on the Volume Mode Run screen (for further information see "<u>Tube Calibration</u>" on page 3-8).
- If required, prime the pump before operation (for further information see "<u>Priming the Pump Drive</u>" on page 3-7).

To record a fluid volume:

- 1. Tap VOLUME from the Mode Selection screen. The Volume Mode Run screen will be displayed.
- 2. Tap EDIT 🖊 to access the Volume Mode Edit screen.
- 3. Tap RECORD (). The Record Dispense screen will be displayed.
- 4. Tap FLOW RATE to make adjustments to the flow rate. The Flow Rate screen will be displayed.
 - a. Tap FLOW to enter the desired flow rate using the onscreen keypad.
 - b. Tap UNITS to enter the desired flow rate units using the onscreen keypad.
 - c. Tap CONFIRM **v** to save changes and return to the Record Dispense screen.
- 5. Tap START ▶ . The drive will now begin pump operation while recording the fluid volume.
- 6. If required, adjustments can be made to flow rate during operation. To make adjustments:
 - a. Tap STOP **and then repeat steps 4–6 above.**
 - b. Tap START > to complete the pump operation once the desired changes have been made.

NOTE: If required, tap STOP and then CANCEL × to discard recording and return to the Volume Mode Edit screen.

- 7. Tap STOP when the desired volume of fluid has been pumped. The recorded dispense volume will now be displayed under VOLUME.
- 8. Tap CONFIRM 🗹 to save or CANCEL 🗙 to discard recording and return to the Volume Mode Edit screen. If saved, the recorded dispense volume will now be displayed under VOLUME.
- 9. Tap CONFIRM 🗹 . The Volume Mode Run screen will be displayed.

REMOTE MODE



CAUTION: Power must be turned off before connecting the external remote control cable to prevent damage to the drive.


The REGLO Digital Pump Drive features both digital remote control and monitoring through the MasterflexLive[™] website using an Ethernet or Wi-Fi connection and/or analog remote control and monitoring via the pump drive's DB-25 female connection port. See <u>www.masterflex.com</u> for more information.

During remote operation:

- The Remote Mode Run screen will be displayed on the pump drive's touchscreen.
- All touchscreen functions, with the exception of STOP ■, SCREEN LOCK 🖻 🖨 and EDIT 🖍 will be disabled.

Remote Mode Run Screen

The Remote Mode Run screen displays the currently selected operation dispense settings (Continuous, Time or Volume) from an external remote control device. The Remote Mode Run screen is accessed by selecting REMOTE from the Mode Selection screen.

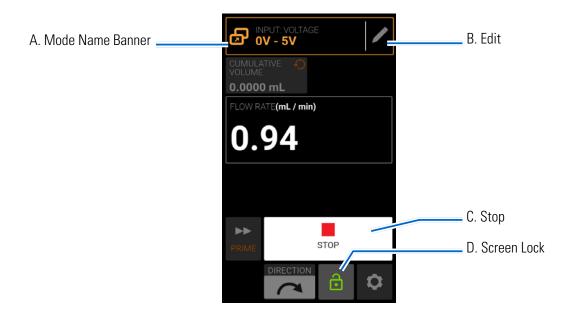

- A. MODE NAME BANNER: Displays the Mode Name as well as the currently selected remote type (ANALOG CURRENT, ANALOG VOLTAGE or MASTERFLEXLIVE[™]). Tap the Mode Name Banner to return to the Mode Selection screen.
- B. EDIT: Tap to access the Remote Mode Edit screen. From the Remote Mode Edit screen adjustments can be made to analog inputs and outputs for voltage and current (for further information see "<u>Analog Input</u>" on page 3-31).

- C. START/STOP/PAUSE: During operation, the display will change from START ► to PAUSE II STOP/ RESET .
- D. SCREEN LOCK: Locking the screen disables all touchscreen functions. **To lock the screen:** Press and hold UNLOCKED in until the icon changes to LOCKED in and a red border appears around the screen. **To unlock the screen:** Press and hold LOCKED in until the icon changes to UNLOCKED in .

Using MasterflexLive[™]

MasterflexLive[™] can be accessed from any suitable digital device connected to the internet, such as a laptop, tablet, smartphone or desktop computer.

General Preparation:

- Confirm the correct tubing has been selected and is properly loaded into the pump drive (for further information see "Loading Tubing" on page 3-3).
- Confirm all fluids and containers are ready.
- Confirm that the tubing has been calibrated by checking that Calibration Complete \$\$\$\$ is displayed on the Remote Mode Edit screen (for further information see "<u>Tube Calibration</u>" on page 3-8).
- If required, prime the pump before operation (for further information see "<u>Priming the Pump Drive</u>" on page 3-7).
- Confirm that the pump drive is connected to the internet via an active Wi-Fi or Ethernet connection.

To connect to MasterflexLive[™]:

- 1. Go to <u>www.masterflex.com</u> and type MasterflexLive into the search bar.
- 2. Follow the onscreen prompts to log in or create a new account.
- 3. Follow the onscreen prompts to add your REGLO pump drive. **NOTE:** The Device ID (listed as the MAC Address) and Device Model Number can be found under "<u>Device Information</u>" on page 3-14. The MAC Address is also located on a label on the pump drive.
- 4. Select the desired pump drive from the list of available devices.
- 5. The Device Remote Control page will be displayed.

- Once the pump drive is connected to MasterflexLive[™] the pump drive can be operated and monitored through the Device Remote Control page and adjustments can be made to any of the pump settings.
- While using MasterflexLive[™] the Remote Mode Run screen will be displayed on the pump drive's touchscreen and local touchscreen control will be unavailable, with the exception of STOP ■, SCREEN LOCK 1 and EDIT
- Tap STOP on the pump drive touchscreen to override the remote control device and immediately stop the pump operation. **NOTE:** If locked, the screen will need to be unlocked before the pump operation can be stopped.
- To lock the screen: Press and hold UNLOCKED i until the icon changes to LOCKED i and a red border appears around the screen. To unlock the screen: Press and hold LOCKED i until the icon changes to UNLOCKED i. NOTE: Stop is disabled when the screen is locked.

Analog Input



CAUTION: Power must be turned off before connecting the external remote control cable to prevent damage to the drive.

The REGLO supports and controls analog input using suitable equipment through the pump drive's DB-25 female connection port. Analog input can be used in place of, or in addition to, MasterflexLive[™].

See also "DB-25 Electrical Connections" on page 3-40.

General Preparation:

- Confirm the correct tubing has been selected and is properly loaded into the pump drive (for further information see "Loading Tubing" on page 3-3).
- Confirm all fluids and containers are ready.
- Confirm that the tubing has been calibrated by checking that Calibration Complete 🇳 is displayed on the Remote Mode Edit screen (for further information see "<u>Tube Calibration</u>" on page 3-8).
- If required, prime the pump before operation (for further information see "<u>Priming the Pump Drive</u>" on page 3-7).
- Confirm that the pump drive is connected to the appropriate equipment through the drive's DB-25 female connection port.

To operate analog control and monitoring:

- 1. Tap REMOTE from the Mode Selection screen. The Remote Mode Run screen will be displayed.
- 2. Tap EDIT 🖌 . The Analog Input screen will be displayed.
- 3. Tap the desired analog input type from the available list.
- 4. If using either ANALOG: VOLTAGE or ANALOG: CURRENT:
 - a. Select the desired current or voltage operating range from the available list.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to cancel and return to the previous screen.

- Tap STOP on the pump drive touchscreen to override the remote control device and immediately stop the pump operation. **NOTE:** If locked, the screen will need to be unlocked before the pump operation can be stopped.
- To lock the screen: Press and hold UNLOCKED i until the icon changes to LOCKED i and a red border appears around the screen. To unlock the screen: Press and hold LOCKED i until the icon changes to UNLOCKED i. NOTE: Stop is disabled when the screen is locked.
- See <u>www.masterflex.com</u> for further information on using analog remote control and monitoring.

Saving Remote Mode Settings as a New Program

Changes made to mode parameters can be saved as a new program for easier access to frequently used mode settings.

To save mode parameters to a new program:

- 1. If required, edit the Remote Mode settings as desired.
- 2. Tap MODE NAME BANNER to return to the Mode Selection screen.
- 4. Tap REMOTE. The Remote New Program screen will be displayed with the last settings used in the Remote Mode.
- 5. Tap PROGRAM1. If required, delete the characters using the back arrow on the onscreen keypad and then enter the desired program name (up to 8 characters).
- 6. Tap CONFIRM to save or DELETE to cancel.

- Once saved, new programs are added in alphabetical order to the bottom of the Mode Selection screen.

CUSTOM PROGRAM MODES

Custom programs allow users to create easily accessible programs for frequently used pump mode settings.

Adding a New Program: Continuous Mode

To add a new Continuous Mode program:

- 2. Tap CONTINUOUS. The Continuous New Program screen will be displayed.
- 3. Tap PROGRAM1. If required, delete the characters using the back arrow on the onscreen keypad and then enter the desired program name (up to 8 characters).
- 4. Select the desired flow rate and flow units:
 - a. Tap FLOW RATE to access the Flow Rate screen.
 - b. Tap UNITS to access the Flow Units screen and select the desired flow unit from the available list.
 - c. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Flow Rate screen.
 - d. Tap FLOW and enter the desired flow rate using the onscreen keypad.
 - e. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Continuous New Program screen.
- 5. Tap SIZE. The Tube Size screen will be displayed.
 - a. Select the desired tube size from the available list or SCROLL imes and tap CUSTOM to enter a custom tube size using the onscreen keypad.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Continuous New Program screen.
- 6. Tap DIRECTION to select either clockwise
 r or counterclockwise
 flow direction.
- 7. Tap CONFIRM to save or DELETE to discard changes.

NOTE:

- Once saved, new programs are added in alphabetical order to the bottom of the Mode Selection screen.

Adding a New Program: Time Mode

To add a new Time Mode program:

- 2. Tap TIME. The Time New Program screen will be displayed.
- 3. Tap PROGRAM1. If required, delete the characters using the back arrow on the onscreen keypad and

then enter the desired program name (up to 8 characters).

- 4. Tap ON TIME to set the amount of time for each pump operation. The On Time Edit screen will be displayed.
 - a. Tap HR, MIN, SEC or TENTHS and enter the desired time using the onscreen keypad.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Time New Program screen.
- 5. Tap OFF TIME to set the amount of time the pump will pause between each operation. The Off Time Edit screen will be displayed. **NOTE:** If the off time is set to 0 (zero) the pump drive will require a start input (from either the touchscreen or a wired input) to start the next dispense.
 - a. Tap HR, MIN, SEC or TENTHS and enter the desired time using the onscreen keypad.
 - b. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Time New Program screen.
- 6. Tap FLOW RATE. The Flow Rate Edit screen will be displayed.
 - a. Tap UNITS to access the Flow Units screen and select the desired flow unit from the available list.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the previous screen.
 - c. Tap FLOW and enter the desired flow rate using the onscreen keypad.
 - d. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Time New Program screen.
- 7. Tap SIZE. The Tube Size screen will be displayed.

 - b. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Time New Program screen.
- 8. Tap DIRECTION to select either clockwise
 or counterclockwise
 flow direction.
- 9. Tap BATCH TOTAL to adjust the number of dispenses in each batch cycle. The Batch Total screen will be displayed.
 - a. Enter the desired number of dispenses in a batch using the onscreen keypad. **NOTE:** If required, tap INFINITE **oo** to select an infinite number of dispense cycles. If infinite is selected, the pump will run continuously.
 - b. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Time New Program screen.

10. Tap CONFIRM to save or DELETE to discard changes.

- Once saved, new programs are added in alphabetical order to the bottom of the Mode Selection screen.

Adding a New Program: Volume Mode

To add a new Volume Mode program:

- 2. Tap VOLUME. The Volume New Program screen will be displayed.
- 3. Tap PROGRAM1. If required, delete the characters using the back arrow on the onscreen keypad and then enter the desired program name (up to 8 characters).
- 4. Tap VOLUME. The Dispense Volume screen will be displayed.
 - a. Tap VOLUME and enter the desired volume using the onscreen keypad. **NOTE:** If the volume of fluid is unknown the pump drive can record fluid dispense volumes (for further information see "<u>Volume Record</u>" on page 3-27).
 - b. Tap RAMP UP \checkmark to set the time the pump takes to reach full flow rate (between 0 and 60 seconds) using the onscreen keypad.
 - c. Tap RAMP DOWN **to** set the time the pump takes to stop at the end of each dispense operation (between 0 and 60 seconds) using the onscreen keypad.
 - d. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Volume New Program screen.
- 5. Tap INTERVAL TIME to set the amount of time the pump will pause between each operation. The Interval Time screen will be displayed. **NOTE:** If the interval time is set to 0 (zero) the pump drive will require a start input (from either the touchscreen or a wired input) to start the next dispense.
 - a. Tap HR, MIN, SEC or TENTHS and enter the desired time using the onscreen keypad.
 - b. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Volume New Program screen.
- 6. Tap FLOW RATE. The Flow Rate Edit screen will be displayed.
 - a. Tap UNITS to access the Flow Units screen and select the desired flow unit from the available list.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the previous screen.
 - c. Tap FLOW and enter the desired flow rate using the onscreen keypad.
 - d. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Volume New Program screen.
- 7. Tap SIZE. The Tube Size screen will be displayed.

 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Volume New Program screen.
- 8. Tap DIRECTION to select either clockwise
 r or counterclockwise
 flow direction.
- 9. Tap BATCH TOTAL to adjust the number of dispenses in each batch cycle. The Batch Total screen will be displayed.

- a. Enter the desired number of dispenses in a batch using the onscreen keypad. **NOTE:** If required, tap INFINITE **oo** to select an infinite number of dispense cycles. If infinite is selected, the pump will run continuously.
- b. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Volume New Program screen.
- 10. If required, tap ANTI-DRIP. The Anti-Drip screen will be displayed (for further information see "<u>Anti-Drip</u>" on page 3-27).
 - a. Tap ON or OFF to enable or disable the Anti-Drip feature.
 - b. If enabled, enter the desired degrees of reverse rotation using the onscreen keypad. **NOTE:** Typical values range from 5 to 45 degrees.
 - c. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Volume New Program screen.
- 11. Tap CONFIRM to save or DELETE to discard changes.

NOTE:

- Once saved, new programs are added in alphabetical order to the bottom of the Mode Selection screen.

Adding a New Program: Remote Mode

To add a new Remote Mode program:

- 2. Tap REMOTE. The Remote New Program screen will be displayed.
- 3. Tap PROGRAM1. If required, delete the characters using the back arrow on the onscreen keypad and then enter the desired program name (up to 8 characters).
- 4. Tap INPUT. The Remote Type screen will be displayed.
- 5. Tap the desired remote type from the available list.
- 6. If using either ANALOG: VOLTAGE or ANALOG: CURRENT:
 - a. Select the desired current or voltage operating range from the available list.
 - b. Tap CONFIRM 🔽 to save or CANCEL 🗙 to cancel and return to the Remote New Program screen.
- 7. Tap SIZE. The Tube Size screen will be displayed.

 - b. Tap CONFIRM 🗸 to save or CANCEL 🗙 to discard changes and return to the Remote New Program screen.
- 8. Tap DIRECTION to select either clockwise
 or counterclockwise
 flow direction.

9. Tap CONFIRM to save or DELETE to discard changes.

NOTE:

- Once saved, new programs are added in alphabetical order to the bottom of the Mode Selection screen.

Using Program Modes

Custom programs will appear in alphabetical order at the bottom of the Mode Selection screen. If there are multiple programs tapping SCROLL ¥ will display additional pages.

General Preparation:

- Confirm the correct tubing has been selected and is properly loaded into the pump drive (for further information see "Loading Tubing" on page 3-3).
- Confirm all fluids and containers are ready.
- Confirm that the tubing has been calibrated by checking that Calibration Complete 🛷 is displayed on the Program Information (i) screen (for further information see "<u>Tube Calibration</u>" on page 3-8).
- If required, prime the pump before operation (for further information see "<u>Priming the Pump Drive</u>" on page 3-7).

To use a program:

- 1. Select the desired program from the Mode Selection screen. The Program Run screen will be displayed.
- 2. Tap START > to begin the pump drive operation using the displayed program settings.
- 3. If required, Tap PAUSE II or STOP during operation. **NOTE:** The pump cannot be paused during Continuous Mode operation.

NOTE:

- Tap INFORMATION (i) to view the selected program's settings.
- Individual settings cannot be edited from the Program Run screen.

Editing a Program

To edit a program:

- 1. Tap EDIT ✓ located next to the desired program name on the Mode Selection screen (**NOTE:** If there are multiple programs, tap SCROLL ➤ to display additional pages). The Program Edit screen will be displayed.
- 2. Edit the settings for the selected mode as desired. For instructions on editing individual mode settings see:
 - "Adding a New Program: Continuous Mode" on page 3-33.
 - "<u>Adding a New Program: Time Mode</u>" on page 3-33.
 - "<u>Adding a New Program: Volume Mode</u>" on page 3-35.

- "Adding a New Program: Remote Mode" on page 3-36.
- **NOTE:** Once the individual mode settings have been edited and saved the Program Edit screen will be displayed.
- 3. Tap CONFIRM 🔽 to save or CANCEL 🗙 to discard changes and return to the Mode Selection screen.

Deleting a Program

To delete a program:

- 1. Tap EDIT ✓ located next to the desired program name on the Mode Selection screen (**NOTE:** if there are multiple programs tap SCROLL imes to display additional pages). The Program Edit screen will be displayed.
- 2. Tap DELETE PROGRAM 🖬 .
- 3. Tap DELETE to delete the program and return to the Mode Selection screen or CANCEL to return to the previous screen.

SECTION 4: SERVICE & MAINTENANCE

CAUTION: Replace the power cord only with one of the same type and rating.

CLEANING THE PUMP DRIVE

If required, the pump drive may be wiped clean using a soft cloth lightly moistened with either isopropyl or ethyl alcohol.

NOTE:

- Do not use water, chlorine or any perfumed or aromatic cleaning agents on the pump drive.
- Care should be taken with the pump drive's touchscreen to avoid scratching or otherwise damaging the surface. Do not wipe with dry or abrasive material.
- Do not operate the pump drive with water on the surface of the touchscreen.
- Any damage caused by improper cleaning will be the sole responsibility of the customer.

SOFTWARE & FIRMWARE UPDATES

Visit <u>www.masterflex.com</u> to download the latest software and firmware updates for your device. **NOTE:** All updates must be downloaded onto a USB drive before installing onto the pump drive.

To install updates:

- 1. Insert the USB drive containing the updates into the pump drive's USB port.
- 2. Tap SETTINGS O from any of the mode screens. The Settings screen will be displayed.
- 4. Tap DEVICE INFORMATION.
- 5. Tap CHECK FOR UPDATES and follow the onscreen prompts.

RESTORE FACTORY SETTINGS

NOTE: Factory reset will erase all settings, including custom programs.

To restore the pump to the original factory defaults:

- 1. Tap SETTINGS O from any of the mode screens. The Settings screen will be displayed.
- 3. Tap DEVICE INFORMATION.
- 4. Tap FACTORY RESET and follow the onscreen prompts.

DB-25 ELECTRICAL CONNECTIONS



CAUTION: Power must be turned off before connecting the external remote control cable to prevent damage to the drive.

13 1 6 3 2 (12) (11) 10 (9) 8 (7) 5 (4) 25 (19) 18 (17) 16 15 14 20 24 23 22 21

Pin No. DB-25	Description	Pin No. DB-25	Description
1	Speed Control Voltage Input (0-10 V)	14	Speed Signal Voltage Output (0-10 V)
2	Speed Control Current Input (0-20 mA)	15	Remote Start/Stop Input
3	Speed Control Input Reference	16	Remote CW/CCW Input
4	Speed Signal Current Output (0-20 mA)	17	Remote Start/Stop, CW/CCW, Prime Reference
5	Speed Signal Output Reference	18	Tach Output Reference
6	Motor Running Relay Output (N.O.)	19	Tach Output (Open Collector)
7	Motor Running Relay Output Common	20	Remote Prime Input
8	Open Head Sensor Relay Output (N.O.)	21	General Alarm Relay Output Common
9	Not Used	22	Not Used
10	Open Head Sensor Relay Output Common	23	General Alarm Relay Output (N.O.)
11–13	Not Used	24–25	Not Used

MINIFLEX PUMP HEAD REPLACEMENT

If necessary, the Miniflex pump head can be replaced. Contact Technical Assistance (see "<u>Technical Assistance</u>" on page 3-48) to order the appropriate replacement pump head.


Description:	Part Number
Replacement Miniflex Single Channel Pump Head	77220-20
Replacement Miniflex Dual Channel Pump Head	77220-30

General preparation and required equipment:

- Confirm you have the correct replacement pump head.
- Remove the pump head from its packaging and inspect for any obvious signs of damage.
- A Phillips head screwdriver is required to remove the pump head fastening screws.

To replace the Miniflex pump head:

- 1. Turn the pump head handle counterclockwise to raise the upper section of the pump head.
- 2. Remove the two fastening screws on the pump head's back plate and carefully remove the pump head.
- 3. Place the new pump head securely onto the Miniflex pump drive.
- 4. Replace the two fastening screws to secure the new pump head to the drive.
- 5. Load tubing and run a dispense calibration to confirm the new pump head is operating correctly (for further information see "Loading Tubing" on page 3-3, and "Tube Calibration" on page 3-8).

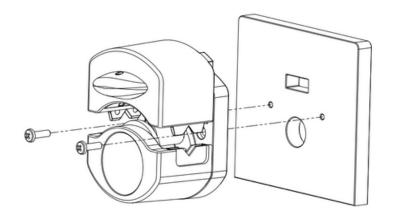

TROUBLESHOOTING

For further assistance, or for issues that cannot be resolved, see "Technical Assistance" on page 3-48.

Symptom Cause		Remedy		
Motor does not rotate.	No power.	1. Check that the power cord is securely plugged into the drive.		
Display does not light.		2. Check that the power cord is plugged into the mains power outlet and that the power is switched on.		
		3. Check the power cord for any visible signs of damage and replace if defective.		
Pump does not rotate	Defective remote control	1. Switch the pump drive off.		
during remote operation. The display does not light up during remote	or setting error.	2. Check that the DB-25 connection cable is fully inserted into the drive's port.		
operation.		3. Switch on the pump drive.		
		4. If the motor still does not rotate, select REMOTE from the Mode Selection screen and/or the Settings screen and verify that the settings are correct.		
		5. For further information see " <u>Remote Mode</u> " on page 3-29.		
Weak calibration strength displayed on the calibra- tion strength bar.	Poor calibration volume and/or flow rate.	Calibration accuracy can be improved by using a larger calibra- tion volume and/or altering the flow rate.		
Touchscreen unrespon- sive.	Wearing thick latex gloves can make the screen less responsive.	Remove gloves before using the touchscreen.		

ERROR DEFINITIONS

	coder Pulses		
Description:	The drive's processor has not received expected encoder feedback.		
Actions:	Drive will stop immediately. Verify load is correct and power cycle drive. If error persists see " <u>Technical Assistance</u> " on page 3-48.		
Error #3: Excee	ded Average Motor Current Limit		
Description:	Motor is drawing too much current on average for a period of time.		
Actions:	Drive will stop immediately. Verify that pump head is not binding and that the load is not above recommended maximum load. If error persists see " <u>Technical Assistance</u> " on page 3-48.		
Error #4: Excee	ded Peak Motor Current		
Description:	Motor is drawing too much current for a short duration of time.		
Actions:	Drive will stop immediately. Verify that pump head is not binding and that the load is not above recommended maximum load. If error persists see "Technical Assistance" on page 3-48.		
Error #5: Comm	unication Watchdog Timeout		
Description:	Internal communications have exceeded allowable time limit.		
Actions:	Drive will stop immediately. Power cycle the pump drive. If error persists see " <u>Technical Assistance</u> " on page 3-48.		
Error #6: Pump	Head Opened During Cal		
Description:	The occlusion bed of the pump is no longer in its closed position, or an internal connection is loose or broken.		
Actions:	Drive will stop immediately. Close pump head. If necessary power cycle the pump drive. If error persists see " <u>Technica</u> <u>Assistance</u> " on page 3-48.		
Error #7: Motor	Over Temperature		
Description:	The pump's temperature sensor has failed or internal temperatures have exceeded limits.		
Actions:	Drive will stop immediately. If necessary remove drive from high ambient temperature, decrease load, and verify that there is free airflow around the drive. If error persists see " <u>Technical Assistance</u> " on page 3-48.		
Error #8: Motor	Direction – Leads Incorrect		
Description:	The motor wires are reversed.		
Actions:	Drive will stop immediately. Power cycle the pump drive. If error persists see "Technical Assistance" on page 3-48.		
Error #9: Over \$	Speed		
Description:	The drive has exceeded commanded speed value.		
Actions:	Drive will stop immediately. Verify load is correct and power cycle the pump drive. If error persists see " <u>Technical</u> <u>Assistance</u> " on page 3-48.		
Error #10: Enco	der Commutation		
Description:	The drive's internal speed sensor is not providing a consistent output.		
Actions:	Drive will stop immediately. Verify load is correct and power cycle the pump drive. If error persists see " <u>Technical</u> <u>Assistance</u> " on page 3-48.		
Error #11: Cal:	Bad Checksum in EEPROM		
Description:	Bad EEPROM checksum for Factory Cal.		
Actions:	Error will be cleared after 10 seconds and parameters will be reset to default values. If error persists see " <u>Technical</u> <u>Assistance</u> " on page 3-48.		

ACCESSORIES

REGLO Accessories

To purchase accessories or for further information visit <u>www.masterflex.com</u>. The following accessories are available for the REGLO Digital Pump Drive:

Description	Part Number	
Footswitch with 6 ft (1.8 m) cable and DB-25 male connector	07523-92	
DB-25 male connector (no cable, connector only)	07523-94	
Cable assembly (DB-25 male connector and 25 ft (7.9 m) cable with stripped wire ends	07523-95	
Dispensing Wand with 6 ft (1.8 m) cable and DB-25 male connector	07523-97	
Power Supply	116065	

Cassettes

Available cassettes for use with the following REGLO pump drive models: 78018-10, 78018-12, 78018-14, 78018-20, 78018-22, and 78018-24.

Description	Part Number
IS3510A Click'n'go POM-C	78016-98
IS0649A Pressure Lever POM-C	07624-64
IS3629A Pressure Lever PVDF	07624-96

Color-Coded Three-Stop Tubing

Color-Coded Three-Stop Tubing suitable for use with cassettes:

 Color-Coded Stops	MM ID
ORANGE/BLACK/ORANGE	0.13
ORANGE/RED/ORANGE	0.19
ORANGE/BLUE/ORANGE	0.25
WHITE/BLUE/WHITE	0.28
RED/BLUE/RED	0.31
BROWN/BLUE/BROWN	0.33
BROWN/BLACK/BROWN	0.36
ORANGE/GREEN/ORANGE	0.38
GREEN/YELLOW/GREEN	0.44
ORANGE/YELLOW/ORANGE	0.51
WHITE/YELLOW/WHITE	0.57
ORANGE/WHITE/ORANGE	0.64
BLACK/BLACK/BLACK	0.76
ORANGE/ORANGE/ORANGE	0.89
WHITE/BLACK/WHITE	0.95
WHITE/WHITE/WHITE	1.02
WHITE/RED/WHITE	1.09
RED/RED/RED	1.14
RED/GRAY/RED	1.22
GRAY/GRAY/GRAY	1.33
YELLOW/YELLOW/YELLOW	1.42
YELLOW/BLUE/YELLOW	1.52
BLUE/BLUE/BLUE	1.65
BLUE/GREEN/BLUE	1.75
GREEN/GREEN/GREEN	1.85
PURPLE/PURPLE/PURPLE	2.06
PURPLE/BLACK/PURPLE	2.29
PURPLE/ORANGE/PURPLE	2.54
PURPLE/WHITE/PURPLE	2.79
BLACK/WHITE/BLACK	3.17

SPECIFICATIONS

OUTPUT			
	Speed:	160 RPM Models	0.15 to 160 RPM
		350 RPM Models	0.18 to 350 RPM
	Torque Output, Max Continuous:	All Models	90 oz-in
	Speed Regulation:	All Models	Line ±0.1% F.S.
			Load ±0.1% F.S.
			Drift ±0.1% F.S.
	Display:	All Models	800 x 480 LCD w/ LED Backlight
	Remote Outputs:	All Models	Voltage speed output (0-10 VDC @ 1 k Ω min)
			Current speed output (4-20 mA @ 0-600 Ω)
			Motor running relay (Closed when running, 1 A max @ 24 VDC)
			General alarm relay (Closed when error is displayed, 1 A @ 24 VDC)
			Open head relay (Closed when activated, 1 A @ 24 VDC)
		160 RPM Models	Tach output (1.5 – 1600 Hz, 50% Duty Cycle, 10 Hz per RPM)
		350 RPM Models	Tach output (1.5 – 3500 Hz, 50% Duty Cycle, 10 Hz per RPM)
INPUT			
	Supply Voltage Limits:	All Models	90 to 260 Vrms @ 50/60 Hz (Universal Input)
	Max Current:	All Models	1.3 A @ 115 VAC; 0.6 A @ 230 VAC
	Remote Inputs:	All Models	Start/Stop, Prime, CW/CCW (Contact closure)
			Current input (0-20 mA @ 249 Ω ; ± 50 V common mode range)
			Voltage input (0-10 VDC @ 10 k $\Omega;\pm$ 50 V common mode range)
			RJ45 Ethernet USB, Type A (5 VDC @ 0.5 A)

CONSTRUCTION			
	Dimensions (L x W x H):	Drive Only	7.62" x 5.75" x 6.31" (194 mm x 146 mm x 160 mm)
	Weight:	Drive Only	5.74 lbs. (2.60 kg)
	Enclosure Rating:	All Models	IP31 per IEC 60529
ENVIRONMENT			
	Operating Temperature:	All Models	0 °C to 40 °C (32 °F to 104 °F)
	Storage Temperature:	All Models	-25 °C to 65 °C (-13 °F to 149 °F)
	Humidity (Non- Condensing):	All models	10% to 90%
	Altitude:	All Models	Less than 2000 m
	Pollution Degree:	All models	Pollution Degree 2 (Indoor use, lab, office)
	Chemical Resistance:	All Models	Exposed material is painted aluminum and ABS plastic
COMPLIANCE			
		All Models	UL 61010-1 US/CAN For CE mark: EN61010-1, Low Voltage Directive EN61326-1, EMC Directive EN50581, RoHS Directive
		Pump Head	EN809, Machinery Directive

TECHNICAL ASSISTANCE

If you have any questions about the use of this product contact the manufacturer or authorized seller.

PRODUCT RETURN

Like all pumps, the REGLO pump drive contains components that will wear over a period of time. To limit charges and delays contact the seller or manufacturer for authorization and shipping instructions before returning the product, either within or outside of the warranty period. When returning the product please state the reason for the return. For your protection, pack the product carefully and insure it against possible damage or loss. Any damages resulting from improper packaging are your responsibility.

WARRANTY

Visit <u>www.masterflex.com</u> for warranty information.

DISPOSAL

Please retain packaging materials until the product warranty ends. Afterwards please discard of any packaging materials in an environmentally friendly manner and according to local regulations.

Once the useful life of the product has ended, please ensure proper disposal according to local laws. Plastic and electronic components should be disposed of at a recycling facility. Please refer to local regulations regarding proper disposal.







US & Canada only Toll Free 1-800-MASTERFLEX | 1-800-637-3739 Outside US & Canada 1-847-549-7600 | 1-847-381-7050 *EN809 manufactured by:

Cole-Parmer Instrument Company 28W092 Commercial Avenue, Barrington, IL 60010 techinfo@masterflex.com | www.masterflex.com